

REC'D 03 FEB 2005

WIPO

EC7

7B/2005/050404

10/591532

PA 1274827

THE UNITED STATES OF AMERICA

TO ALL TO WHOM THESE PRESENTS SHALL COME:

UNITED STATES DEPARTMENT OF COMMERCE

United States Patent and Trademark Office

January 21, 2005

THIS IS TO CERTIFY THAT ANNEXED HERETO IS A TRUE COPY FROM THE RECORDS OF THE UNITED STATES PATENT AND TRADEMARK OFFICE OF THOSE PAPERS OF THE BELOW IDENTIFIED PATENT APPLICATION THAT MET THE REQUIREMENTS TO BE GRANTED A FILING DATE UNDER 35 USC 111.


APPLICATION NUMBER: 60/542,259 ✓

FILING DATE: February 05, 2004 ✓

PRIORITY DOCUMENT

SUBMITTED OR TRANSMITTED IN
COMPLIANCE WITH RULE 17.1(a) OR (b)

By Authority of the
COMMISSIONER OF PATENTS AND TRADEMARKS

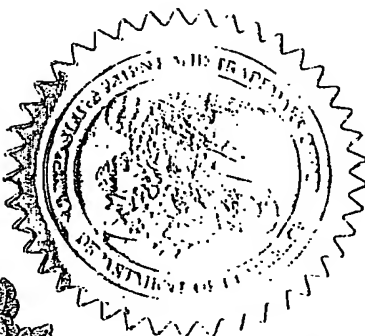

M. SIAS

Certifying Officer

17296 U.S. PTO

Please type a plus sign (+) inside this box → ☒

Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

PTO/SB/16 (02-01)

Approved for use through 10/31/2002. OMB 0851-0032
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE

PROVISIONAL APPLICATION FOR PATENT COVER SHEET

This is a request for filing a PROVISIONAL APPLICATION FOR PATENT under 37 CFR 1.53(c).

Express Mail Label No. EU778901063US

020504
60542259
U.S. PTO

INVENTOR(S)					
Given Name (first and middle (if any))	Family Name or Surname	Residence (City and either State or Foreign Country)			
Matthew	Bruce	Seattle, WA			
Jeffrey E.	Powers	Bainbridge Island, WA			
David	Hope Simpson	Bothell, WA			
<input checked="" type="checkbox"/> Additional inventors are being named on the <u>1</u> separately numbered sheets attached hereto					
TITLE OF THE INVENTION (280 characters max)					
ULTRASONIC IMAGING OF PERFUSION AND BLOOD FLOW WITH HARMONIC CONTRAST AGENTS					
Direct all correspondence to:					
<input checked="" type="checkbox"/> Customer Number		28159		Place Customer Number Bar Code Label here	
OR Type Customer Number here					
<input type="checkbox"/> Firm or Individual Name		W. Brinton Yorks, Jr.			
Address					
Address					
City		State	ZIP		
Country		Telephone	425-487-7152	Fax	
ENCLOSED APPLICATION PARTS (check all that apply)					
<input checked="" type="checkbox"/> Specification		Number of Pages	21	<input type="checkbox"/> CD(s), Number	
<input checked="" type="checkbox"/> Drawing(s)		Number of Sheets	4	<input checked="" type="checkbox"/> Other (specify)	Express Mail Certificate Receipt Confirmation Postcard
<input type="checkbox"/> Application Data Sheet. See 37 CFR 1.76					
METHOD OF PAYMENT OF FILING FEES FOR THIS PROVISIONAL APPLICATION FOR PATENT					
<input type="checkbox"/> Applicant claims small entity status. See 37 CFR 1.27.				FILING FEE AMOUNT (\$)	
<input type="checkbox"/> A check or money order is enclosed to cover the filing fees				160.00	
<input checked="" type="checkbox"/> The Commissioner is hereby authorized to charge filing fees or credit any overpayment to Deposit Account Number:		14-1270			
<input type="checkbox"/> Payment by credit card. Form PTO-2038 is attached.					
The invention was made by an agency of the United States Government or under a contract with an agency of the United States Government.					
<input checked="" type="checkbox"/> No.					
<input type="checkbox"/> Yes, the name of the U.S. Government agency and the Government contract number are:					

Respectfully submitted,

SIGNATURE

W. Brinton Yorks, Jr.

TYPED or PRINTED NAME

W. Brinton Yorks, Jr.

TELEPHONE

425-487-7152

Date 5 Feb 2004

REGISTRATION NO.
(if appropriate)
Docket Number:

28,923

PHUS040117

USE ONLY FOR FILING A PROVISIONAL APPLICATION FOR PATENT

This collection of information is required by 37 CFR 1.51. The information is used by the public to file (and by the PTO to process) a provisional application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.14. This collection is estimated to take 8 hours to complete, including gathering, preparing, and submitting the complete provisional application to the PTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, Washington, D.C. 20231. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. SEND TO: Box Provisional Application, Assistant Commissioner for Patents, Washington, D.C. 20231.

PROVISIONAL APPLICATION COVER SHEET **Additional Page**

PTO/SB/16 (02-01)
 Approved for use through 10/31/2002. OMB 0651-0032
 U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE

Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

Docket Number		PHUS040117	Type a plus sign (+) inside this box →	+
INVENTOR(S)/APPLICANT(S)				
Given Name (first and middle (if any))	Family or Surname	Residence (City and either State or Foreign Country)		
Michalakis	Averkiou	Kirkland, WA		

Number 1 of 1

WARNING: Information on this form may become public. Credit card information should not be included on this form. Provide credit card information and authorization on PTO-2038.

ULTRASONIC IMAGING OF PERFUSION AND BLOOD FLOW
WITH HARMONIC CONTRAST AGENTS

5 This invention relates to ultrasonic diagnostic
imaging systems and, in particular, to the use of
ultrasonic imaging to segment and visualize perfusion
of tissue and blood vessel flow with ultrasonic
contrast agents.

10 Ultrasonic diagnostic imaging has benefited from
the enhancement of perfusion studies and blood flow
imaging with harmonic contrast agents for a number of
years. In a typical study the contrast agent is
introduced into the patient intravenously.
15 Ultrasonic imaging is then commenced at a region of
interest such as the heart or blood vessels. As the
injected bolus of contrast agent begins arriving at
the region of interest the microbubbles of the
contrast agent return relatively strong ultrasonic
20 echoes. Furthermore, these echo signals have
significant nonlinear (e.g., second harmonic)
components. Detecting signals at the second harmonic
of the transmit frequency thus produces signals from
the contrast agent which dominate those returned by
other reflectors in the body. An image which maps
25 the locations of the contrast agent in the body thus
reveals the locations of the blood flow which carries
the microbubbles, and images produced from the second
harmonic signals and other harmonic components
segment out the locations of blood flow to the
30 relative exclusion of the surrounding tissue.

The use of contrast agents to image the
perfusion of microvasculature in tissues such as the
myocardium or liver has been found to produce
excellent results which enable various techniques for
35 quantifying the perfusion of tissue with a flow of

ATL-356

blood. As used herein, the term "perfusion" relates to the amount of blood flow per volume of tissue. With the advent of low power (low MI) contrast agents and techniques, a single dose of contrast agent can provide a relatively long period during which the contrast agent is present in the body and perfusing the tissue. However, such long imaging periods are generally not prevalent when imaging and diagnosing larger blood vessels. The larger arterial blood vessels will usually begin to fill first following the bolus injection of the contrast agent and can initially be imaged with good results. But in time the contrast agent will begin to fill the microvasculature of the surrounding tissue, obscuring the flow of contrast agents in the larger vessels. One technique for dealing with this problem is to image at a higher MI which is just high enough to continuously destroy the slower moving microbubbles in the microvasculature of the region of interest while continuing to visualize the faster moving microbubbles in the larger vessels. This approach will reduce the effective imaging time because the contrast agent is constantly being destroyed. Furthermore, it is often difficult to adjust and maintain the appropriate transmit power levels in a clinical environment to maintain the constant destruction of microvasculature microbubbles without significantly disrupting those in the larger vessels. It would be desirable to be able to image both contrast agent tissue perfusion and the flow of contrast agents in the larger vessels simultaneously as both provide significant useful clinical information. But it is desirable to do so in a way which affords substantial contrast agent imaging time

ATL-356

to enable the most comprehensive and accurate diagnosis of the patient.

5 In accordance with the principles of the present invention, an ultrasonic diagnostic imaging system and method are described which provide the simultaneous imaging of both tissue perfusion and larger vessel blood flow by contrast agents. Multiple, differently modulated transmit signals are used to acquire ensembles of echo information from 10 points within a region of interest. The ensembles are differently filtered to produce contrast agent signals characteristic of perfusion and/or higher velocity blood flow. The ultrasound system uses these signals to produce an image of the blood flow in larger vessels against a background of tissue 15 perfusion. The clinician is thus able to visualize tissue perfusion and larger vessel flow simultaneously with the larger vessel flow clearly segmented against the perfusion background.

20 In the drawings:

FIGURE 1 illustrates in block diagram form an ultrasound system constructed in accordance with the principles of the present invention.

25 FIGURE 2 is a detailed block diagram of the contrast signal filtering of the detection and classification of ultrasound signals from different sources in the ultrasound system of FIGURE 1.

FIGURES 3a-3c illustrate the characteristics of the filters of FIGURE 2.

30 FIGURE 4a-4b illustrate response characteristics useful for classifying the received signals in the embodiment of FIGURE 2.

35 Referring first to FIGURE 1, an ultrasonic diagnostic imaging system constructed in accordance with the principles of the present invention is shown

ATL-356

in block diagram form. This system operates by scanning a two or three dimensional region of the body being imaged with ultrasonic transmit beams. As each beam is transmitted along its steered path through the body, the tissue and blood flow in the body return echo signals with linear and nonlinear (fundamental and harmonic) components corresponding to the transmitted frequency components. The transmit signals are modulated by the nonlinear effects of the tissue through which the beam passes or the nonlinear response of a contrast agent microbubble encountered by the beam, thereby generating echo signals with nonlinear components.

The ultrasound system of FIGURE 1 utilizes a transmitter 16 which transmits waves or pulses of a selected modulation characteristic in a desired beam direction for the return of harmonic echo components from scatterers within the body. The transmitter is responsive to a number of control parameters which determine the characteristics of the transmit beams as shown in the drawing, including the frequency components of the transmit beam, their relative intensities or amplitudes, and the phase or polarity of the transmit signals. The transmitter is coupled by a transmit/receive switch 14 to the elements of an array transducer 12 of a probe 10. The array transducer can be a one dimensional array for planar (two dimensional) imaging or a two dimensional array for two dimensional or volumetric (three dimensional) imaging.

The transducer array 12 receives echoes from the body containing fundamental and harmonic (nonlinear) frequency components which are within the transducer passband. These echo signals are coupled by the switch 14 to a beamformer 18 which appropriately

ATL-356

delays echo signals from the different transducer elements, then combines them to form a sequence of fundamental and harmonic signals along the beam from shallow to deeper depths. Preferably the beamformer is a digital beamformer operating on digitized echo signals to produce a sequence of discrete coherent digital echo signals from a near field to a far field depth of field. The beamformer may be a multiline beamformer which produces two or more sequences of echo signals along multiple spatially distinct receive scanlines in response to a single transmit beam, which is particularly useful for 3D imaging. The beamformed echo signals are coupled to an ensemble memory 20.

In accordance with one aspect of the present invention, multiple waves or pulses are transmitted in each beam direction using different modulation techniques, resulting in the reception of multiple echoes for each scanned point in the image field. The echoes corresponding to a common spatial location are referred to herein as an ensemble of echoes, and are stored in the ensemble memory 20, from which they can be retrieved and processed together. The echoes of an ensemble are processed in various ways as described more fully below to produce the desired fundamental or harmonic signals. The echo signals are processed by a B mode signal path including a grayscale signal processor 22 and by a Doppler signal path including a Doppler processor 24. In the illustrated embodiment the Doppler processor is provided in an ASIC (application specific integrated circuit) which includes two parallel paths for the processing of two Doppler signals at the same time. These paths are shown as Doppler processor A and Doppler processor B in the drawing.

ATL-356

The grayscale and Doppler processors can be operated individually in the conventional manner to produce a grayscale image or a Doppler image, or a colorflow image which is formed by the overlay of a fundamental or harmonic grayscale tissue image with Doppler flow information. In accordance with the present invention signals from the grayscale and Doppler processors 22 and 24 are coupled to a classifier 30. In a constructed embodiment the classifier is formed by software running on a CPU which analyzes the received signals and decides whether a received signal should be displayed as a pixel in a flow image or a pixel in a perfusion image or both. For example a large vessel may be visualized in both a perfusion image and a flow image. The signal is appropriately stored in an image memory 32 which is partitioned into a flow image section and a perfusion image section. The flow and perfusion images are further processed as by scan conversion and combined in an overlay of the flow image overlaying the perfusion image by an image processor 36. Alternatively the flow information can be embedded in the perfusion image in the image memory. Additionally the flow and perfusion images can overlay an image of the tissue background. The resultant image is displayed on an image display 38.

The vascular flow and/or perfusion images may be alternatively removed via a user control either in review of a Cineloop sequence or during live imaging. This enables the clinician to view the perfusion image over tissue, the flow image over tissue or both tissue and flow together over tissue. It also enables either perfusion or flow to be viewed in isolation from other information. The transparency of the perfusion and flow images can be altered to

ATL-356

enable visualization of perfusion, flow and background tissue images together. For example, when the microcirculation is filled with microbubbles the perfusion image may largely obscure underlying tissue or flow. The perfusion may then be displayed in a semi-transparent mode so that the clinician can view the underlying tissue or flow while still appreciating the tissue perfusion.

In use, an ultrasonic contrast agent is introduced into the patient's vascular system and imaging of a region of interest such as the liver commences at a low MI. Initially, before the contrast agent arrives at the region of interest, a tissue image is formed by signals received from tissue. These signals are processed by a background tissue signal processor in the B mode signal path. The background tissue signal processor produces an image of the background tissue in the region of interest in a manner similar to the processing of the grayscale signal processor 22, but with thresholds set to detect signals from tissue. The tissue signals may be fundamental or harmonic. Generally fundamental signals are preferred when operating at a low MI where tissue harmonic signals will be at low levels. The background tissue image is coupled to the image processor 36 where it is displayed initially as just a tissue image, then as a background to flow and perfusion as the contrast agent begins to fill the region of interest.

The larger arterial vessels in the region of interest will begin to light up first in the image as the contrast agent will arrive in the larger vessels first due to their higher flow velocities. The larger vessels are displayed from the fundamental and harmonic signals produced by flowing contrast agent

ATL-356

and detected by the Doppler processor 24. In time,
the contrast agent will begin to perfuse the tissue
surrounding the larger vessels and the microbubbles
slowly begin to perfuse the microvasculature of the
5 tissue. This filling of the microvasculature with
microbubbles increases the nonlinear signals detected
by the grayscale signal processor. This perfusion of
the tissue will then light up from the nonlinear
(harmonic) amplitude response of the signals produced
10 by the grayscale signal processor. The displayed
image will thus appear as a contrast perfusion image
containing larger vessels of more rapidly flowing
contrast microbubbles. The signal paths A and B of
the Doppler processor 24 are operated at the harmonic
15 and fundamental frequencies respectively. In a
constructed embodiment this fundamental and nonlinear
mixing enables the display of the larger vessels in
the near field as nonlinear (harmonic) contrast
segments and the larger vessels in the far field as
20 linear fundamental contrast segments, thereby
compensating for the attenuation of higher harmonic
frequencies from the deeper depths. The fundamental
and harmonic signals may be blended together into one
flow image, thereby showing larger vessel flow over a
25 considerable depth of field against a background of
perfused tissue.

A variety of different transmit sequences may be
employed to detect the nonlinear signal components.
Harmonic separation is preferably performed by what
30 is known as "pulse inversion," by which the echoes
from multiple, differently modulated transmit pulses
are combined to separate the harmonic components and
attenuate linear fundamental components. The
different modulation may be different phase
35 modulation, polarity modulation, or amplitude

ATL-356

modulation, or a combination thereof as described in
US patent application serial number 60/527538, filed
December 5, 2003 and entitled "ULTRASONIC SPECKLE
REDUCTION USING NONLINEAR ECHO COMBINATIONS." For
5 example, a transmit sequence may comprise three
transmit pulses transmitted at the desired pulse
repetition interval (PRI) for the Doppler flow
velocities being detected, with the first pulse
having a nominal amplitude of 0.5 and a phase or
10 polarity of 0° or +, a second pulse having a nominal
amplitude of 1.0 and a phase or polarity of 180° or -,
and a third pulse having a nominal amplitude of 0.5
and a phase or polarity of 0° or +. When the echoes
from the three transmit pulses are normalized in
15 amplitude and additively combined the linear
fundamental frequency components cancel and the
harmonic components are enhanced. With amplitude and
phase modulation (see US Pat. 6,095,980 (Burns et
al.) and US Pat. 6,319,203 (Averkiou)) it is possible
20 to combine the nonlinear echoes in a way that some
energy at the fundamental frequency is present. This
energy is referred to herein as "nonlinear
fundamental" energy and it is the result of the
harmonic activity at unequal amplitudes. The
25 "nonlinear fundamental" should not be confused with
the linear response of a system with a single
excitation at the fundamental frequency. The
nonlinear fundamental can be used in both the
detection of perfusion and/or the detection of
30 vascular flow. Alternatively, pairs of differently
modulated pulses transmitted at a rapid rate to
prevent motion artifacts can be transmitted at the
PRI from one pulse pair to the next as described in
US patent 6,620,103 (Bruce et al.), which shows how
35 the pulse pairs can be spatially interleaved over

ATL-356

different transmit lines for low velocity flow detection.

5 A detailed diagram of the grayscale and Doppler processors is shown in FIGURE 2. The echo signals from an ensemble of transmit pulses 1-N are applied to the inputs of the processors. The grayscale signal path 22 includes a quadrature bandpass filter (QBP) 42, which passes harmonic echo signals in a band around $2f_0$. Construction and operation of a quadrature bandpass filter is described in US Pat. 10 6,050,942 (Rust et al.) which explains how the filter produces the I and Q components of an echo signal in a desired passband. These components of an echo ensemble are further filtered by the lowpass characteristic of a matrix wall filter, which passes 15 echoes returned from tissue and stationary microbubbles. The matrix wall filter may exhibit a response characteristic such as that illustrated in FIGURE 3a. The low pass filter response is seen to 20 roll off at $PRF/2$, half the repetition frequency of the echo ensemble. For the case of pulse inversion, fundamental frequency echo signals from tissue or stationary microbubbles are contained in a band 62 located at the end of the passband, since the QBP is 25 operating in the harmonic band. Harmonic signal components are located in a band 64 at the nominal DC point of the filter response. The filtered ensemble of echoes is applied to an estimator 52 which combines the echo signals to separate the nonlinear 30 second harmonic signal components and detects the signal power or amplitude squared. This signal path functions in the manner of a nonlinear pulse inversion processor to pass nonlinear signals from stationary or nearly stationary microbubbles which 35 have perfused tissue in the region of interest.

ATL-356

The second signal path 24A in this embodiment is a Doppler processing path which includes a QBP 42b set to pass harmonic frequencies. This could be the same QBP as used in the grayscale signal path or could be a separate QBP as shown in the drawing. The signals passed by QBP 42b are filtered by a bandpass matrix wall filter 46. This filter is designed to detect harmonic flow signals as there is considerable overlap of fundamental and harmonic components produced by the QBP when broadband transmit pulses are used. Nonlinear pulsing schemes other than phase or polarity modulated pulse inversion (e.g., combinations of phase or polarity pulse inversion and amplitude modulation) may be used in a similar fashion to detect both perfusion and flow of contrast agents and to separate linear and nonlinear components even in the case of broadband transmit signals. A response characteristic useful for this first Doppler signal path is shown in FIGURE 3b. The bandpass characteristic 70,70' is seen to have a stop band at DC. The fundamental frequencies from microbubbles are located as shown at 72, and at 74 for moving microbubbles, attenuated by the QBP 42b. Harmonic signal components from stationary microbubbles are located in a band 76 at the stop band of the filter, and detectable signals from moving microbubbles are located in the band 78. The filtered harmonic flow signal ensemble is coupled to an estimator 54 which estimates the harmonic flow signals. These signals will exhibit good axial and lateral resolution due to the high harmonic frequencies and will exhibit good signal-to-clutter ratios since the echoes from flowing microbubbles are significantly stronger than returned tissue harmonic signals. These echoes will thus provide good spatial

ATL-356

resolution by comparison with the blooming effect which can be seen with fundamental frequency flow detection. Further details of harmonic Doppler processing can be found in US Pat. 6,036,643 (Criton et al.), which is in the context of tissue harmonic Doppler.

The third signal path 24B includes a QBP 42c set to pass fundamental frequencies f_0 . The fundamental frequency ensemble passed by this QBP is filtered by a matrix wall filter 48 with a band pass characteristic such as that shown in FIGURE 3c. Harmonic components in the vicinity of the stop band 76 are attenuated, aided by the QBP response and depth-dependent attenuation, as are echo signals from stationary components in band 72 at the filter skirt. Moving microbubbles will exhibit a relatively strong response in band 74. These echo signal components will have a good signal-to-noise ratio in comparison to harmonic signals, but will have a lower signal-to-clutter response and exhibit relatively low spatial resolution since strong fundamental frequency echo signals are returned by both tissue and microbubbles. Image segments using these echoes can exhibit some blooming due to the high sensitivity of detection and signal-to-noise ratio of the Doppler signal estimator 56. Consequently, in a preferred embodiment, flow in the near field utilizes the harmonic Doppler flow signals produced by path 24A. At deeper depths where the harmonic frequencies become attenuated, the fundamental Doppler flow signals are used for display. At intermediate depths the flow display is a blend of the harmonic and fundamental signals, making a varying ratio transition from 100% harmonic to 100% fundamental over a transition depth region. The blending of harmonic and fundamental signals with

ATL-356

depth is described in US Pat. 6,283,919 (Roundhill et al.) Thus, flow can be shown in the perfusion and flow image over a considerable depth of view.

The signals produced by the three processing paths 22, 24A, and 24B are classified for use as tissue, stationary microbubbles (perfusion) or flowing microbubbles (in larger vessels) by the classifier 30. This classification could be done on the basis of the power and velocity estimates of the wall filtered signals. In the illustrated embodiment the classifier decides the image(s) in which to display the echoes in response to a velocity variance estimation path which includes a QBP 42d operating at the fundamental frequency f_0 , and a velocity variance processor 50. As shown by the dashed line at the output of the velocity variance processor, these variance estimates may also be classified and used for display. The variance estimate is computed as the root mean square of the Doppler velocity bandwidth, which, to a first order approximation, can be estimated using an equation of the form $1 - \frac{|R(1)|}{|R(0)|}$, where $R(0)$ is the echo value squared and can be computed by

$$R(0) = \frac{1}{N} \sum_{n=1}^N x(n)x^*(n)$$
 and $R(1)$ is the magnitude of the first lag of the autocorrelation of the echo values and can be computed by

$$R(1) = \frac{1}{N} \sum_{n=1}^N x(n)x^*(n-1).$$
 Using velocity for signal segmentation is premised on the assumption that tissue and microbubbles in microvasculature (perfusion) move at relatively low velocities and exhibit a relatively narrow dispersion of velocities, and microbubbles in larger vessels move at relatively

ATL-356

higher velocities and exhibit a relatively wider dispersion of velocities. A segmentation scheme such as that shown in FIGURE 4a can be used by the classifier 30 in response to calculations of mean velocity. This scheme has two curves 82 and 84 which divide the response into different regions. If, for instance, a velocity estimate $R(o)$ for a pixel exhibits relatively low mean velocity (Doppler frequency) $\langle f \rangle$ and relatively high power, it is likely that the signal came from tissue and it will be displayed in the perfusion image. These velocity estimates will be in the region defined generally by the area 86. Those signals exhibiting higher mean velocities $\langle f \rangle$ and relatively lower power are likely from flow, and signals classified generally in the area 88 will be displayed in the Doppler flow image.

Another classification scheme which is predicated on variance estimates is shown in FIGURE 4b. Estimates $R(o)$ with relatively narrow (low) velocity variance and relatively significant power in area 92 are likely lower velocity perfusion microbubbles in the microvasculature of tissue and will be displayed in the perfusion image. Estimates $R(o)$ which have somewhat less power but exhibit a broader (higher) velocity variance in area 94 are likely from flowing microbubbles and will be displayed in the flow image. Signals below the variance threshold 98 are classified as from tissue with or without microbubbles in its microcirculation. Signals below the amplitude or power threshold 96 are classified as noise which exhibits broad, random variance.

Thus it is seen that both perfusion and blood flow can be segmented and imaged simultaneously for an extended period of time in a single displayed

ATL-356

image by imaging contrast at low MIs and utilizing
the concepts of the present invention.

5

ATL-356

WHAT IS CLAIMED IS:

1. A method of ultrasonically imaging blood perfusion and blood flow in a region of interest of a body comprising:

5 acquiring a sequence of ultrasonic echo signals from a body which has been infused with an ultrasonic contrast agent;

10 processing the echo signals to detect the tissue structure in the absence of microbubbles;

processing a plurality of the echo signals in a first way to detect echo signals returned from tissue microvasculature perfused with the contrast agent;

15 processing a plurality of the echo signals in a second way to detect echoes returned from blood flow containing the contrast agent in larger vessels;

utilizing the echo signals processed the first way to form a portion of an image depicting perfusion;

20 utilizing the echo signals processed the second way to form a portion of an image depicting blood flow in larger vessels; and

25 displaying an ultrasound image depicting both contrast-enhanced perfusion and contrast-enhanced blood flow.

30 2. The method of Claim 1, wherein displaying further comprises depicting both the presence and locations of microbubbles in tissue and the velocity of microbubbles in blood flow.

35 3. The method of Claim 1, further comprising deciding the portion of the image which an echo signal is to form on the basis of a blood flow velocity estimation.

ATL-356

4. The method of Claim 3, wherein deciding further comprises deciding the portion of the image which an echo signal is to form on the basis of a blood flow variance estimation.

5. The method of Claim 1, wherein processing a plurality of echo signals in first and second ways comprises processing the same ensemble of echo signals in first and second ways.

6. The method of Claim 1, wherein acquiring a sequence of ultrasonic echo signals further comprises acquiring an ensemble of echoes over time from each of a plurality of different locations in the body.

7. The method of Claim 1, wherein processing a plurality of the echo signals in a first way comprises detecting the amplitude or power of the echo signals; and wherein processing a plurality of the echo signals in a second way comprises Doppler processing the plurality of the echo signals.

8. The method of Claim 7, wherein processing a plurality of the echo signals in both the first way and the second way both include detecting nonlinear components of the echo signals by the pulse inversion technique.

9. The method of Claim 1, wherein utilizing the echo signals processed the first way further comprises forming a perfusion image; and wherein utilizing the echo signals processed the second way further comprises forming a flow image;

ATL-356

and

wherein displaying an ultrasound image further comprises displaying the perfusion image overlaid with the flow image.

5

10. The method of Claim 1, further comprising transmitting a plurality of differently modulated transmit pulses in each of a plurality of different beam directions;

10

wherein processing a plurality of the echo signals in both the first way and the second way both include detecting harmonic components of the echo signals by the pulse inversion technique.

15

11. An ultrasonic diagnostic imaging system for imaging both perfusion and flow in a body infused with a contrast agent comprising:

20

an ultrasonic transducer array operated to transmit a plurality of pulses in each of a plurality of different beam directions and to receive echoes in response to the pulses;

25

a beamformer coupled to the transducer array;
a first processor coupled to the beamformer and responsive to pluralities of echo signals for detecting echoes returned from perfused tissue;
a second processor coupled to the beamformer and responsive to ensembles of echo signals for detecting echoes returned from blood flow containing contrast in larger vessels;

30

a decision processor, coupled to the first and second processors, for identifying signals to be displayed on the basis of velocity;

35

an image memory responsive to the decision circuit which acts to utilize signals produced by the first and second processors to form a perfusion image

ATL-356

portion and a flow image portion; and

a display coupled to the image memory which displays an ultrasound image which depicts both contrast perfused tissue and the flow in larger vessels in a common image.

5

12. The ultrasonic diagnostic imaging system of Claim 11, wherein the second processor includes a first signal path which Doppler processes nonlinear echo ensembles and a second signal path which Doppler processes fundamental frequency echo ensembles,

10

wherein the display displays an image of nonlinear Doppler processed flow in the near field and fundamental frequency Doppler processed flow in the far field.

15

13. The ultrasonic diagnostic imaging system of Claim 11, further comprising a transmitter, coupled to the transducer array, which acts to transmit a plurality of differently modulated beams in each of a plurality of different beam directions.

20

14. The ultrasonic diagnostic imaging system of Claim 13, wherein each of the first and second processors process harmonic signals separated by the pulse inversion technique.

25

15. The ultrasonic diagnostic imaging system of Claim 11, wherein the decision processor acts to identify signals to be displayed on the basis of velocity variance.

30

16. The ultrasonic diagnostic imaging system of Claim 15, further comprising a velocity variance estimator responsive to echo signals processed by the

35

ATL-356

first and second processors and coupled to the decision processor.

5 17. The ultrasonic diagnostic imaging system of Claim 11, wherein the image memory comprises a first image buffer for storing a perfusion image and a second image buffer for storing a flow image.

10 18. The ultrasonic diagnostic imaging system of Claim 11, further comprising a tissue signal processor which acts to detect echoes from tissue in the absence of microbubbles.

15 19. The ultrasonic diagnostic imaging system of Claim 18, wherein the display acts to selectively display an image which is less than all of the combination of a tissue image component, a perfusion image component, and a flow image component.

20 20. The ultrasonic diagnostic imaging system of Claim 19, further comprising means for adjusting the opacity of one of the image components to be semi-transparent, whereby obscured tissue or flow may be visualized through the semi-transparent image
25 component.

ATL-356


ULTRASONIC IMAGING OF PERFUSION AND BLOOD FLOW
WITH HARMONIC CONTRAST AGENTS

Abstract of the disclosure:

5

10 An ultrasonic diagnostic imaging method and
system produce diagnostic contrast images depicting
both tissue perfusion and flow velocity in larger
vessels by utilizing both linear and nonlinear
imaging techniques. A sequence of echoes from
differently modulated transmit pulses is received and
processed in different ways to detect nonlinear
signals from microbubble-perfused tissue and Doppler
blood flow in larger vessels. The Doppler flow
15 signals may be either linear or nonlinear or a
mixture of both. A decision circuit classifies the
detected signals for display pixels in a perfusion
and/or flow and/or tissue image. Separate perfusion
and flow images can be simultaneously displayed or an
20 image of both perfusion and flow can be displayed.

ATL-356

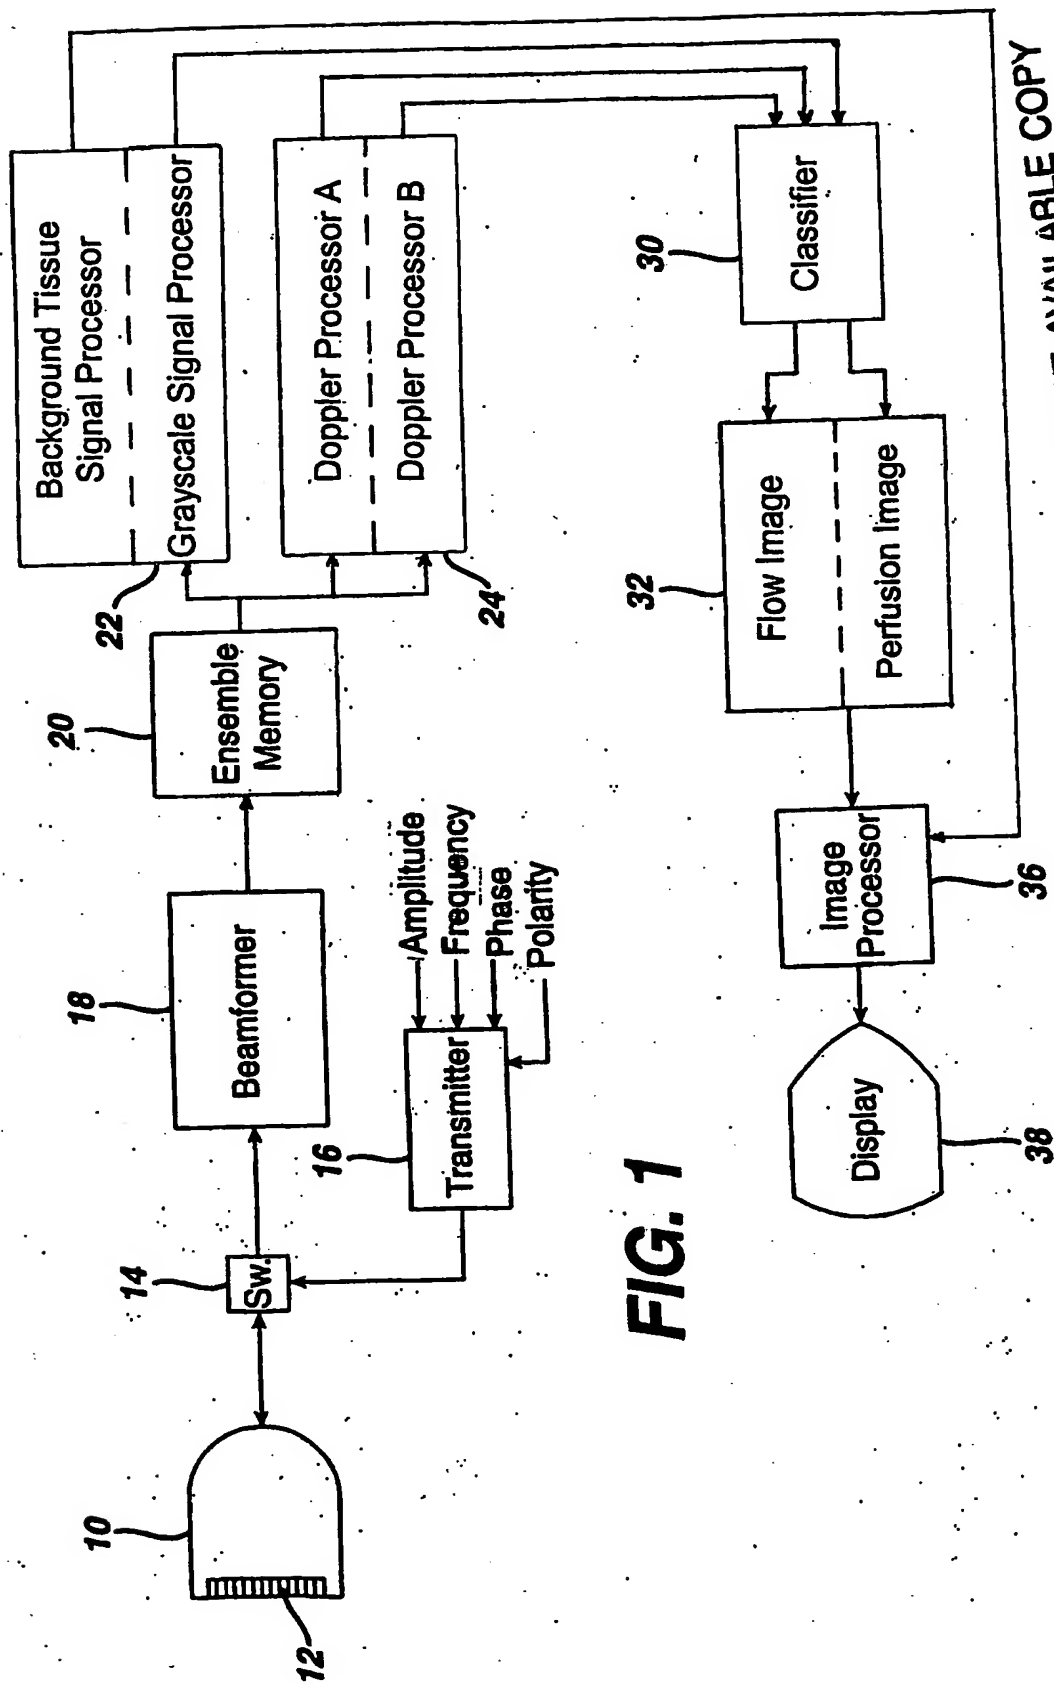

BEST AVAILABLE COPY

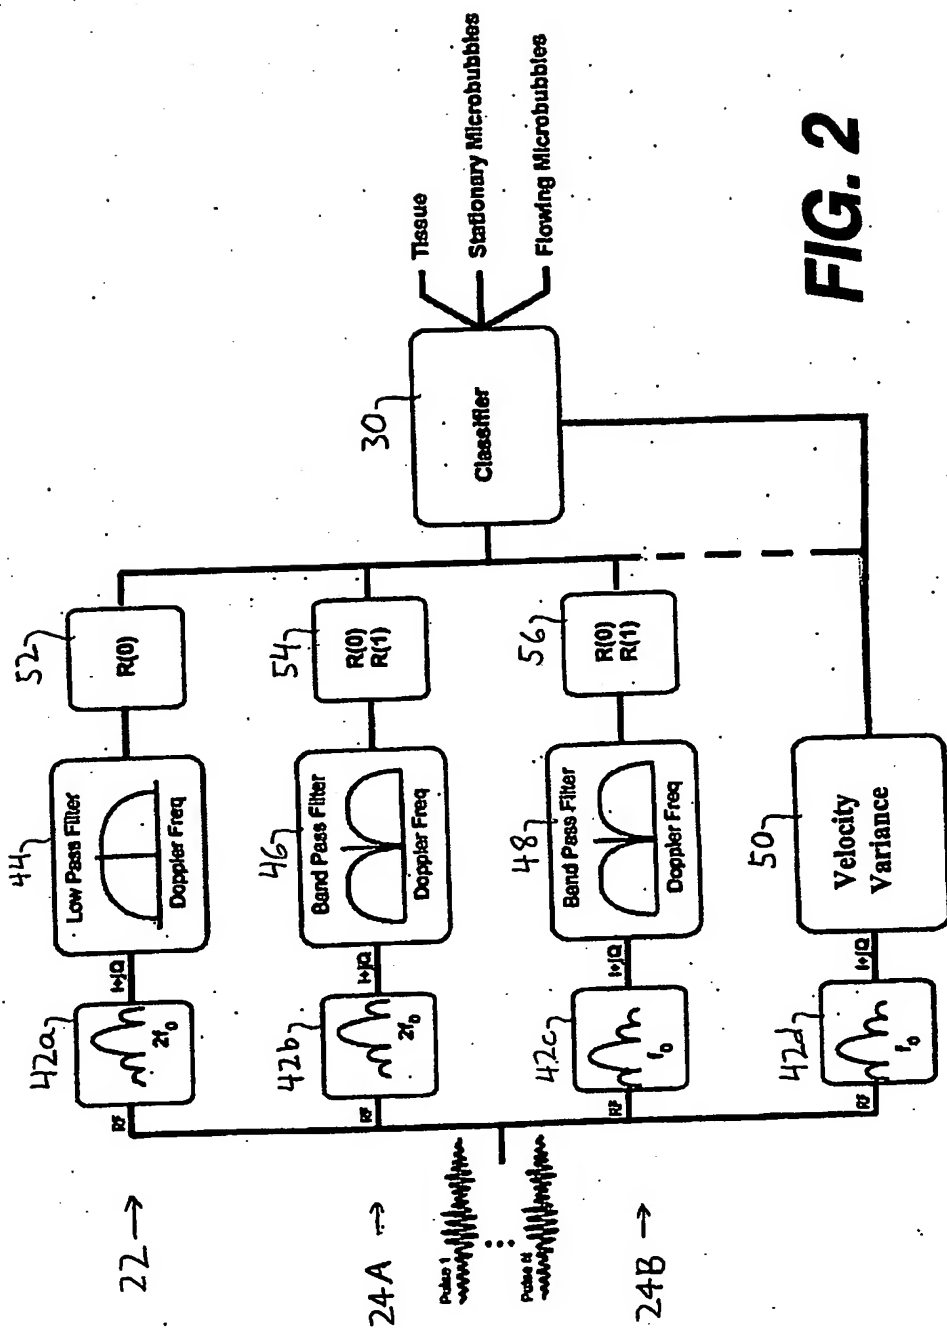
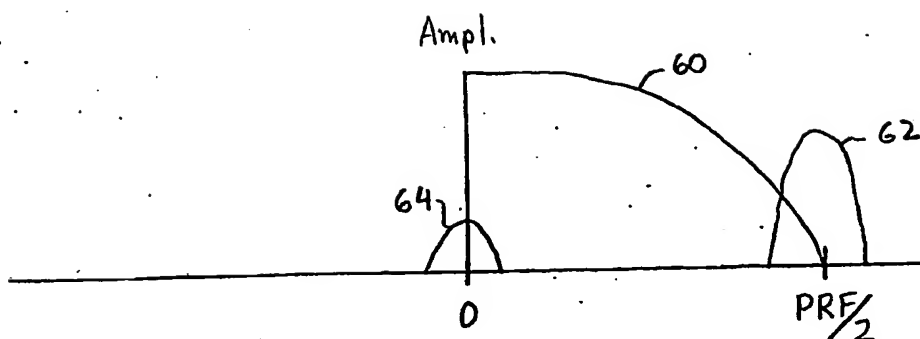
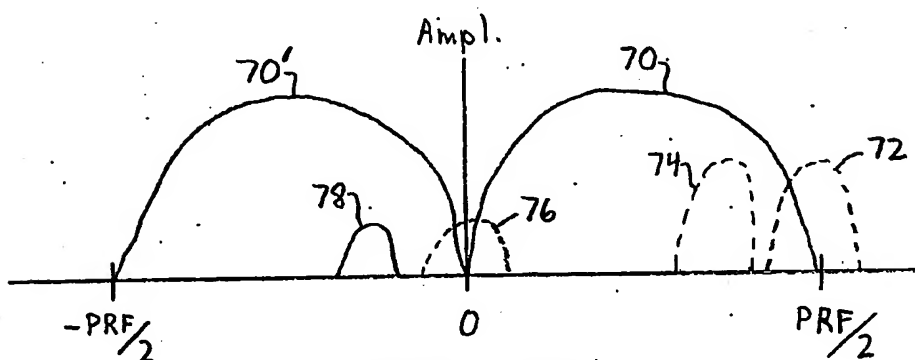
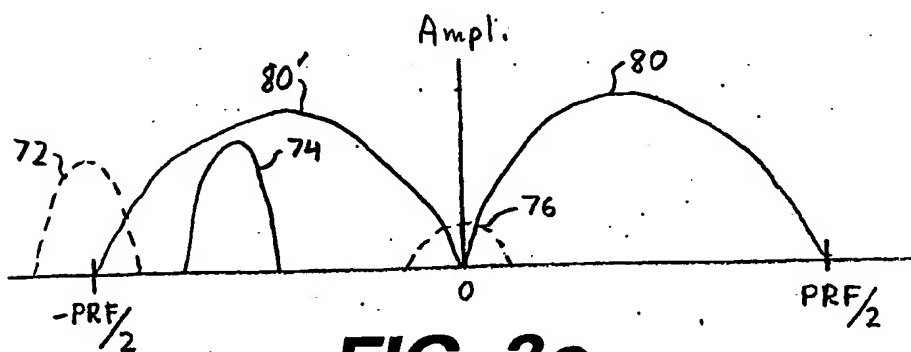


FIG. 2

BEST AVAILABLE COPY

**FIG. 3a****FIG. 3b****FIG. 3c**

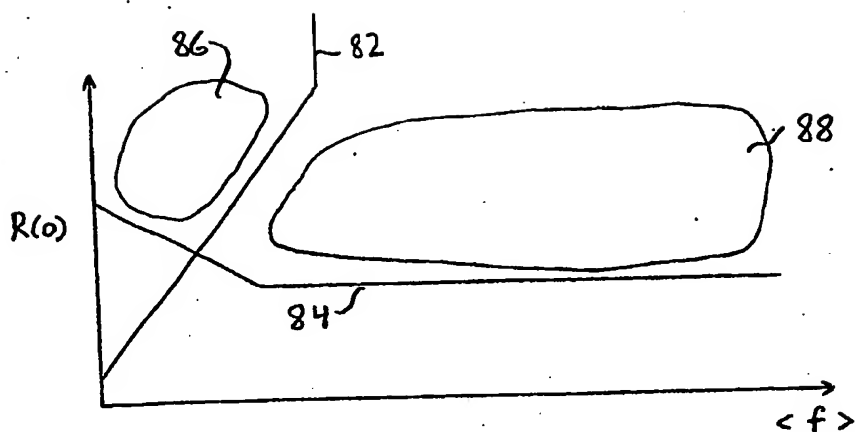


FIG. 4a

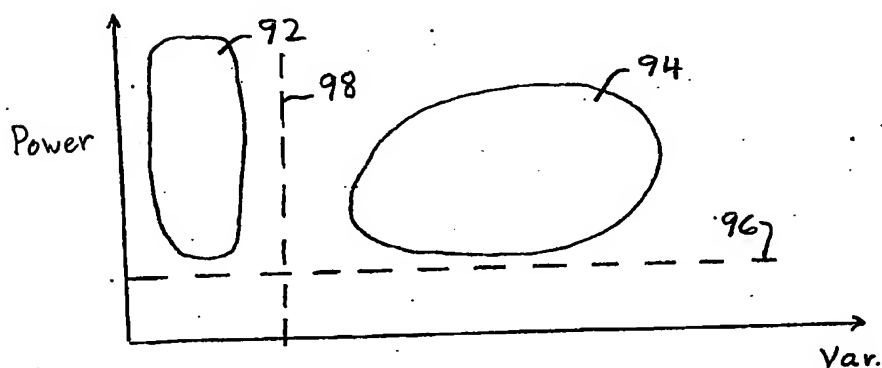


FIG. 4b

BEST AVAILABLE COPY